

HEMOCLOT™ Protein S

REF CK041K-RUO **R1** **R2** 3 x 1 mL

REF CK042K-RUO **R1** **R2** 3 x 2 mL

Clotting method for the measurement of Protein S activity

FOR RESEARCH USE ONLY.

DO NOT USE IN DIAGNOSTIC PROCEDURES.

English, last revision: 01-2021

INTENDED USE:

The HEMOCLOT™ Protein S kit is a clotting method for the *in vitro* quantitative determination of Protein S (PS) activity on citrated human plasma, using a manual or automated method.

This kit is for research use only and must not be used for patient diagnosis or treatment.


SUMMARY AND EXPLANATION:

Technical:

Protein S (PS) is a vitamin K dependent protein, mainly synthesized in liver. Plasma PS exists in two forms: complexed with C4b-BP, or as free form that presents anticoagulant activity by acting as cofactor of Activated Protein C (APC). In the presence of calcium and phospholipids, the APC-PS complex inhibits Factors Va and VIIIa.

PRINCIPLE:

The HEMOCLOT™ Protein S kit is a clotting method, using activated partial thromboplastin time (APTT), triggered by Factor IXa in the presence of phospholipids, calcium and a constant and in excess amount of APC. The diluted test plasma is mixed with PS deficient plasma (R1). The activator reagent (R2), at constant and optimized concentration, is added. Coagulation is triggered by adding calcium (Ca²⁺). Since PS is the limiting factor, this results in a direct relationship between PS concentration and the corresponding measured clotting time.



REAGENTS:

R1 **Protein S deficient plasma**, immuno-depleted, lyophilized in the presence of an heparin neutralizing agent.

R2 **Activator reagent**, lyophilized. Contains human Factor IXa, human APC, and phospholipids, in an optimized concentration. Contains BSA.

REF CK041K-RUO → **R1** **R2** 3 vials of 1 mL

REF CK042K-RUO → **R1** **R2** 3 vials of 2 mL

WARNINGS AND PRECAUTIONS:

- Some reagents provided in these kits contain materials of human and animal origin. Whenever human plasma is required for the preparation of these reagents, approved methods are used to test the plasma for the antibodies to HIV 1, HIV 2 and HCV, and for hepatitis B surface antigen, and results are found to be negative. However, no test method can offer complete assurance that infectious agents are absent. Therefore, users of reagents of these types must exercise extreme care in full compliance with safety precautions in the manipulation of these biological materials as if they were infectious.
- Waste should be disposed of in accordance with applicable local regulations.
- Use only the reagents from the same batch of kits.
- Aging studies show that the reagents can be shipped at room temperature without degradation.
- This device of *in vitro* use is intended for professional use in the laboratory.

REAGENT PREPARATION:

Gently remove the freeze-drying stopper, to avoid any product loss when opening the vial.

R1 **R2** Reconstitute the contents of each vial with exactly:

REF CK041K-RUO → 1 mL of distilled water

REF CK042K-RUO → 2 mL of distilled water

Shake vigorously until complete dissolution while avoiding formation of foam and load it on the analyzer following application guide instruction.

For manual method, allow to stabilize for 15 minutes at room temperature (18-25°C), homogenize before use.

STORAGE AND STABILITY:

Unopened reagents should be stored at 2-8°C in their original packaging. Under these conditions, they can be used until the expiry date printed on the kit.

R1 **R2** Reagent stability after reconstitution, free from any contamination or evaporation, and stored closed, is of:

- 24 hours** at 2-8°C.
- 8 hours** at room temperature (18-25°C).
- Do not freeze.**
- Stability on board of the analyzer: see the specific application.**

REAGENTS AND MATERIALS REQUIRED BUT NOT PROVIDED:

Reagents:

- Distilled water
- Imidazole Buffer (AR021B-RUO/AR021K-RUO/AR021L-RUO/AR021M-RUO/AR021N-RUO)
- CaCl₂ at 0.025M (AR001B-RUO/AR001K-RUO/AR001L-RUO)
- Specific calibrators and controls:

Product name	Reference
BIOPHEN™ Plasma Calibrator	222101-RUO
BIOPHEN™ Normal Control Plasma	223201-RUO
BIOPHEN™ Abnormal Control Plasma	223301-RUO

Use the same buffer for all tests performed.

Also refer to the specific application guide of the analyzer used.

Materials:

- Water-bath, semi-automatic or automatic analyzer for clotting assays.
- Stopwatch; Calibrated pipettes; silicon glass or plastic test tubes.

SPECIMEN COLLECTION AND PREPARATION:

The blood (9 volumes) should be carefully collected onto the trisodium citrate anticoagulant (1 volume) (0.109 M, 3.2%) by clean venipuncture. Discard the first tube.

Specimens should be prepared and stored in accordance with applicable local guidelines (for the United States, see the CLSI H21-A5¹ guideline for further information concerning specimen collection, handling and storage).

For plasma storage, please refer to references ^{1,2}.

PROCEDURE:

The kit can be used in manual or automated method. The assay is performed at 37°C, and the clotting time, triggered by the addition of calcium, is measured.

For an automated method, application guides are available on request. See specific application guide and specific precautions for each analyzer.

Assay method:

1. Reconstitute the calibrator and controls as indicated in the specific instructions. The calibrator should be diluted in Imidazole buffer as described below in order to perform the calibration range ("C" defines the PS concentration or by definition 100% for a normal plasma pool):

When calibration is performed with a commercially available plasma calibrator (e.g. BIOPHEN™ Plasma Calibrator), the **1:10** dilution corresponds to the indicated "C" PS activity concentration.

For a calibrator titrating C, the level of 100% (in the assay conditions) is obtained by diluting this standard by the following factor: **10x(C)/100**.

The calibration range can also be performed using a pool of normal citrated plasma (at least 30 normal individuals, men and women, aged 18 to 55, with no known treatment or pathology), which by definition is at **100%** of PS. The assay incorporates a **1:10** dilution of the plasma, which corresponds by definition to 100% of PS. The calibration range is **0 to 100%** PS.

Prepare **3 mL** of the **1:10** dilution of the normal pool of plasmas, or a dilution (**10x(C)/100**) of the calibrator plasma titrated in PS (i.e. **C1**). This solution corresponds to 100% of PS. Prepare the following calibration range by successive dilutions in the Imidazole buffer as described in the table below in order to perform the calibration range:

Calibrator	C5	C4	C3	C2	C1
Protein S (%)	0%	25%	50%	75%	100%
Volume of calibrator	0 mL	0,250 mL	0,500 mL	0,750mL	1 mL
Volume of imidazole bufer	1 mL	0,750 mL	0,500 mL	0,250mL	0 mL

2. Dilute the samples in imidazole buffer as described in the table below:

Samples	Reference	Dilution
Control	223201-RUO / 223301-RUO	1/10
Samples	N.A.	1/10

For best results, for expected concentrations >100%, values can be obtained by testing plasma at 1:20 dilution and then multiply the results by 2; for sample ≤10%, use 1:5 dilution and divide the result by 2.

Realize the calibration range and test it quickly with the quality controls. Diluted samples should be tested quickly, if stored at room temperature (18-25°C). Whenever possible, for optimal performance, all tests (calibration, samples and controls) should be carried out extemporaneously and simultaneously. The exact concentrations of the calibrators and controls are indicated for each lot on the flyer supplied with the kit.


3. In a plastic tube incubated at 37°C, introduce:

	Volume
Calibrator, control or plasma (diluted)	50 µL
R1 Protein S deficient plasma , preincubated at 37°C	50 µL
Mix and incubate for 1 minute at 37°C, then add:	
R2 Activator reagent , preincubated at 37°C	50 µL
Mix and incubate for 3 minutes at 37°C, then add (starting the stopwatch):	
CaCl ₂ 0.025M (preincubated at 37°C, and stirred)	100 µL
Note the clotting time, in seconds	CT

If a reaction volume different from that indicated above is required for the method used, the volume ratio must be strictly observed in order to guarantee the performance of the assay. The user is responsible for validating changes and their impact on all results.

CALIBRATION:

The HEMOCLOT™ Protein S assay can be calibrated for the functional assay of plasma Protein S. The calibrator covering the calibration range is available from HYPHEN BioMed (see the REAGENTS AND MATERIALS REQUIRED BUT NOT PROVIDED paragraph) and can be used to establish the calibration curve. The calibration range is about 0 to 100% (on STA-R series). The calibration curve shown below is given by way of example only. The calibration curve established for the assay series must be used.

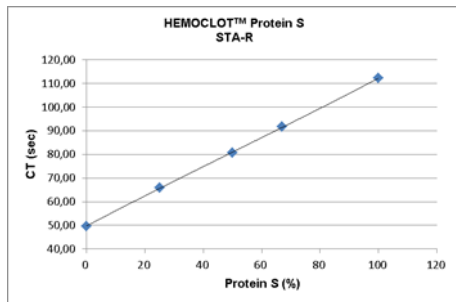

QUALITY CONTROL:

The use of quality controls serves to validate method compliance, along with between-test assay homogeneity for a given batch of reagents. Include the quality controls with each series, as per good laboratory practice, in order to validate the test. A new calibration curve should be established, preferably for each test series, and at least for each new reagent batch, or after analyzer maintenance, or when the measured quality control values fall outside the acceptance range for the method. Each laboratory must define its acceptance ranges and verify the expected performance in its analytical system.

RESULTS:

- For the manual end point method, plot the calibration curve lin-lin, with the clotting time (sec) along the Y-axis and the PS concentration, expressed as %, along the X-axis.
- The concentration of PS (%) in the test specimen is directly inferred from the calibration curve, when the standard dilution is used.
- If other dilutions are used, the level obtained should be multiplied by the additional dilution factor used.

The results obtained should be for research use only and must not be used for patient diagnosis or treatment.

LIMITATIONS:

- To ensure optimum test performance and to meet the specifications, the technical instructions validated by HYPHEN BioMed should be followed carefully.
- Any reagent presenting an unusual appearance or showing signs of contamination must be rejected.

- Any suspicious samples or those showing signs of activation must be rejected.
- If clotting times are shortened or prolonged, the result should be confirmed by another method (e.g. immunological) and / or another sample.
- For a same batch of reagents, and a same plasma, the clotting time (CT) may vary depending on the instrument used (particularly depending on the detection of the clot in mechanical or optical mode) and the adjustment of the clot detection sensitivity.

PERFORMANCES:

- The lower analyzer detection limit depends on the analytical system used (≤ 10% on STA-R®-series).
- The measurement zone depends on the analytical system used (approximately 10 to 100% PS on STA-R®-series, without redilution).
- Specificity: PS deficient plasma measured <5%.
- Performance studies were performed internally on STA-R®. The performances were evaluated with the laboratory controls over 5 days, 2 series per day and 2 repetitions at each series for a control level. The following results were obtained:

Control	Intra-assays				Inter-assays			
	N	Moy.	CV%	SD	n	Moy.	CV%	SD
Samples 1	20	95,5	3,2	3,0	20	98,5	5,2	5,1
Samples 2	20	33,2	7,1	2,4	20	33,2	8,1	2,7

- Interferences:** No interference on the instrument STA-R® has been observed with the molecules and up to the following concentrations:

Intralipids (mg/dL)	Hemoglobin (mg/dL)	Bilirubin (mg/dL)	Heparins (UFH/LMWH) (IU/mL)
1000	100	60	1

Also refer to the specific application guide of the analyzer used.

REFERENCES:

- CLSI Document H21-A5: "Collection, transport, and processing of blood specimens for testing plasma -based coagulation assays and molecular hemostasis assays; approved guideline". 2008.
- Mauge L. and Alhenc-Gelas M. Stabilité pré-analytique des paramètres de la coagulation: revue des données disponibles. Ann Biol Clin. 2014.

SYMBOLS:

Symbols used and signs listed in the ISO 15223-1 standard, see Symbol definitions document.

Changes compared to the previous version.